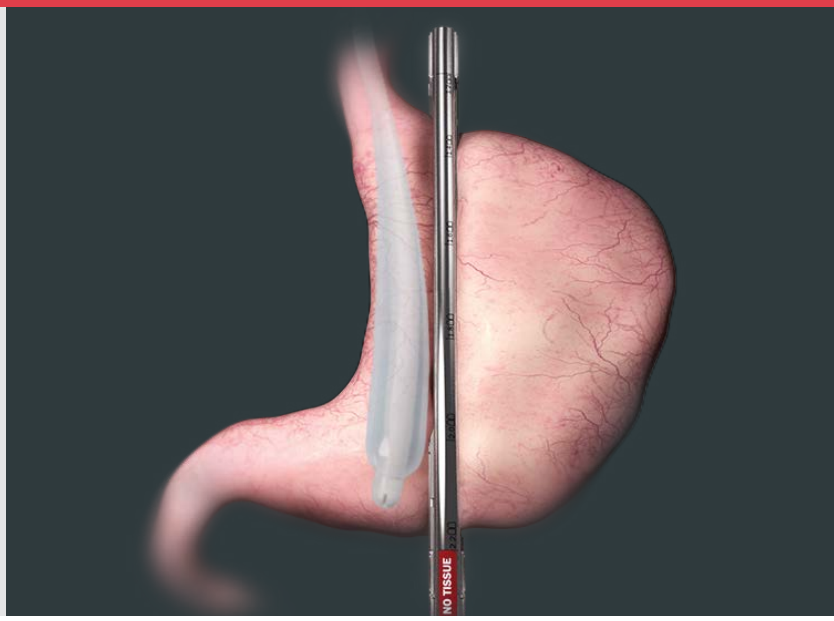
STANDARD BARIATRICS™

# Titan SGS™ Precision Bougie

Designed for use with the Titan SGS™ Stapler

**Precision Matters**

The Titan SGS™ Precision Bougie is designed to achieve precise anatomical alignment and help protect the incisura angularis.[1] Designed for use with the Titan SGS™ Stapler, this device supports a consistent anatomy-based approach to sleeve gastrectomy.



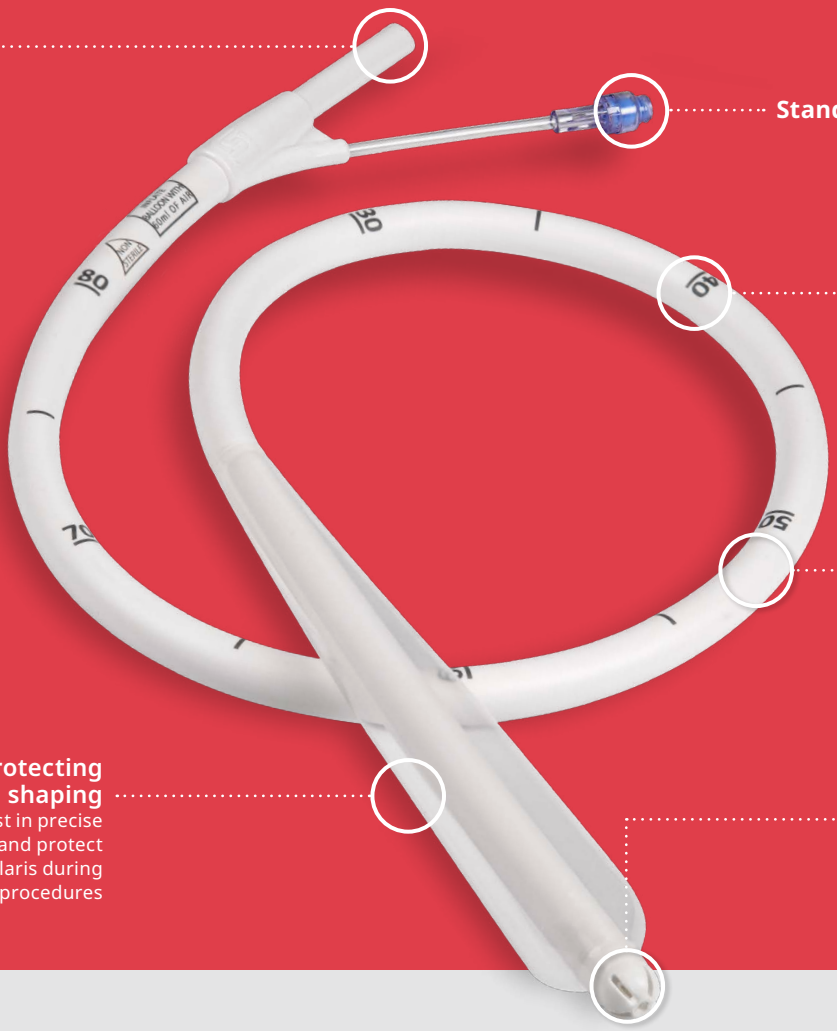

**COMPATIBILITY**
Design optimized to work with the Titan SGS™ Stapler

**PRECISION**
Engineered to achieve precise anatomical alignment and help protect the incisura angularis[1]

**FLEXIBILITY**
Custom blended thermoplastic polyurethane for enhanced manipulability and flexibility

**Scan for more information or visit StandardBariatrics.com**

Teleflex™
Empowering the future of healthcare




## SLEEVE SHAPE MATTERS

### A purpose-built design for an anatomy-based approach

The Titan SGS™ Stapler is the first commercially available stapler in the United States designed specifically for sleeve gastrectomy and engineered to deliver a more consistent, symmetrical sleeve anatomy.[2,3] Featuring the industry's longest 23 cm continuous staple line[3] it streamlines your workflow while standardizing pouch anatomy so you can standardize your operational efficiency and outcomes.



## Titan SGS™ Precision Bougie

| | |
|---|---|
| Order Code | STB38 |
| EA/BX | 6 |
| Tubing | The catheter tubing is approximately 95cm long and has a diameter of 38 French (12.7mm) |
| Drainage Holes | The Titan SGS™ Precision Bougie includes apertures at the tip of the catheter |
| Balloon | The balloon is located 1.9cm from the distal end and is 16.6cm long |
| Syringe | 60mL/CC syringe provided for the purpose of inflating the balloon with air |


1. U.S. Food and Drug Administration. 510(k) Premarket Notification: K222085. Published October 31, 2022.
2. Teleflex Incorporated. Data on File. Search of FDA cleared product code GDW through February 2025.
3. U.S. Food and Drug Administration. 510(k) Premarket Notification: K210278. Published April 28, 2021.


**CAUTION: Federal (USA) law restricts this device to sale or use by or on the order of a physician.**

Information in this material is not a substitute for the product Instructions for Use. Refer to the package insert provided with the product for complete warnings, indications, contraindications, precautions, potential complications and instructions for use.


Teleflex, the Teleflex logo, Standard Bariatrics, and Titan SGS are trademarks or registered trademarks of Teleflex Incorporated or its affiliates, in the U.S. and/or other countries.

Not all products may be available in all countries. Please contact your local representative.

© 2026 Teleflex Incorporated. All rights reserved. MC-011374 Rev 0 05/2026.



**Distributed by:**
**Teleflex** · 3015 Carrington Mill Boulevard, Morrisville, NC 27560
Toll Free: 866 246 6990
**teleflex.com | standardbariatrics.com**


Teleflex™
Empowering the future of healthcare